

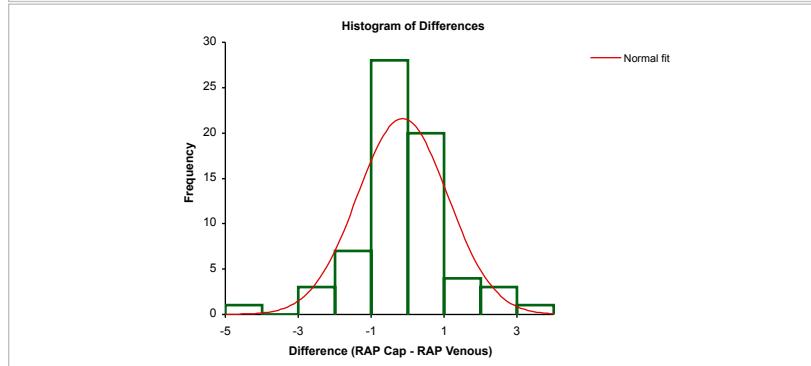


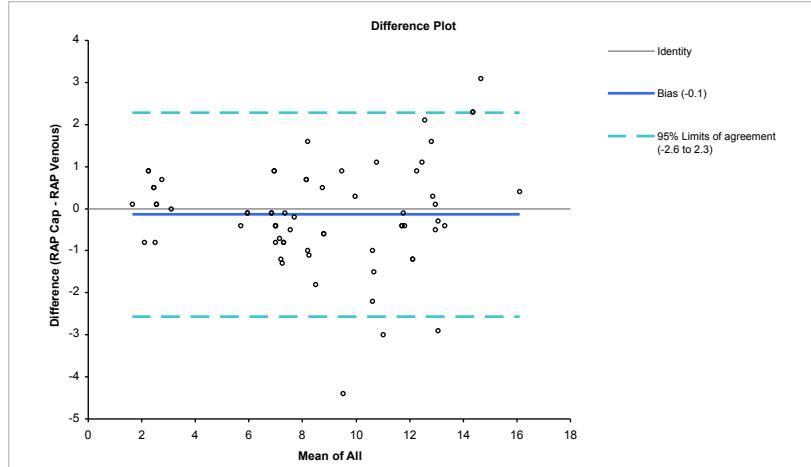

bioscience
Protecting the Gift of Life

Test	Agreement - Altman Bland test	Analyse-it v2.04
Performed by	RAP Venous v RAP Cap	Date
		17 March 2009

n	67
Correlation - absolute difference v average	0.34
Bias	-0.14
95% CI	-0.44 to 0.16
SE	0.151
t statistic	-0.93
DF	66
p	0.3566
SD of differences	1.24 between single measurements
95% Limits of agreement	95% CI
Lower	-2.56
Upper	2.28
	-3.08 to -2.05
	1.77 to 2.80

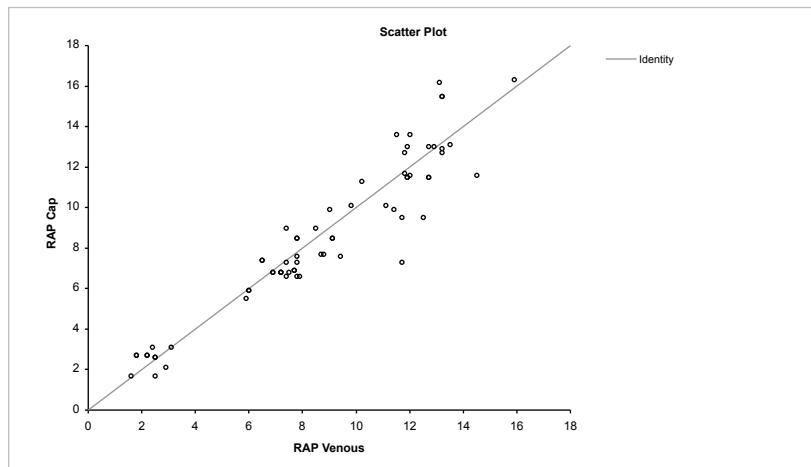

info@tmsbioscience.com
134 LaSalle Street, Suite 4
New Orleans, LA 70112

Phone: 504.962.3377 | Fax: 504.962.3378

TMS BioScience is officially registered as Therapeutic Monitoring Services, L.L.C. © 2009